

Purpose

This procedure defines the policies and related procedures Fluke follows to comply with the requirements of the ISO 9001:2015, ISO/IEC 17025 and ISO/IEC 80079-34 standards.

Introduction

Fluke Corporation (Fluke) is a leading manufacturer of measurement and test equipment with corporate headquarters located in Everett, Washington, USA with global operations and subsidiaries.


Fluke uses a process approach in our Quality Management System (QMS) where required inputs and desired outputs are identified and monitored to ensure applicable requirements and customer expectations are met.



Fluke is part of the Fortive Corporation and employs the [Fortive Business System](#) (FBS) as the cornerstone of our culture and our competitive advantage. FBS drives continuous improvement of our Quality Management System. Tools include Kaizen events, Problem Solving Process (PSP), risk analysis and other tools as appropriate.

Fluke's interaction of processes of the Quality Management System is shown in the following diagram.

Fluke Quality Management System

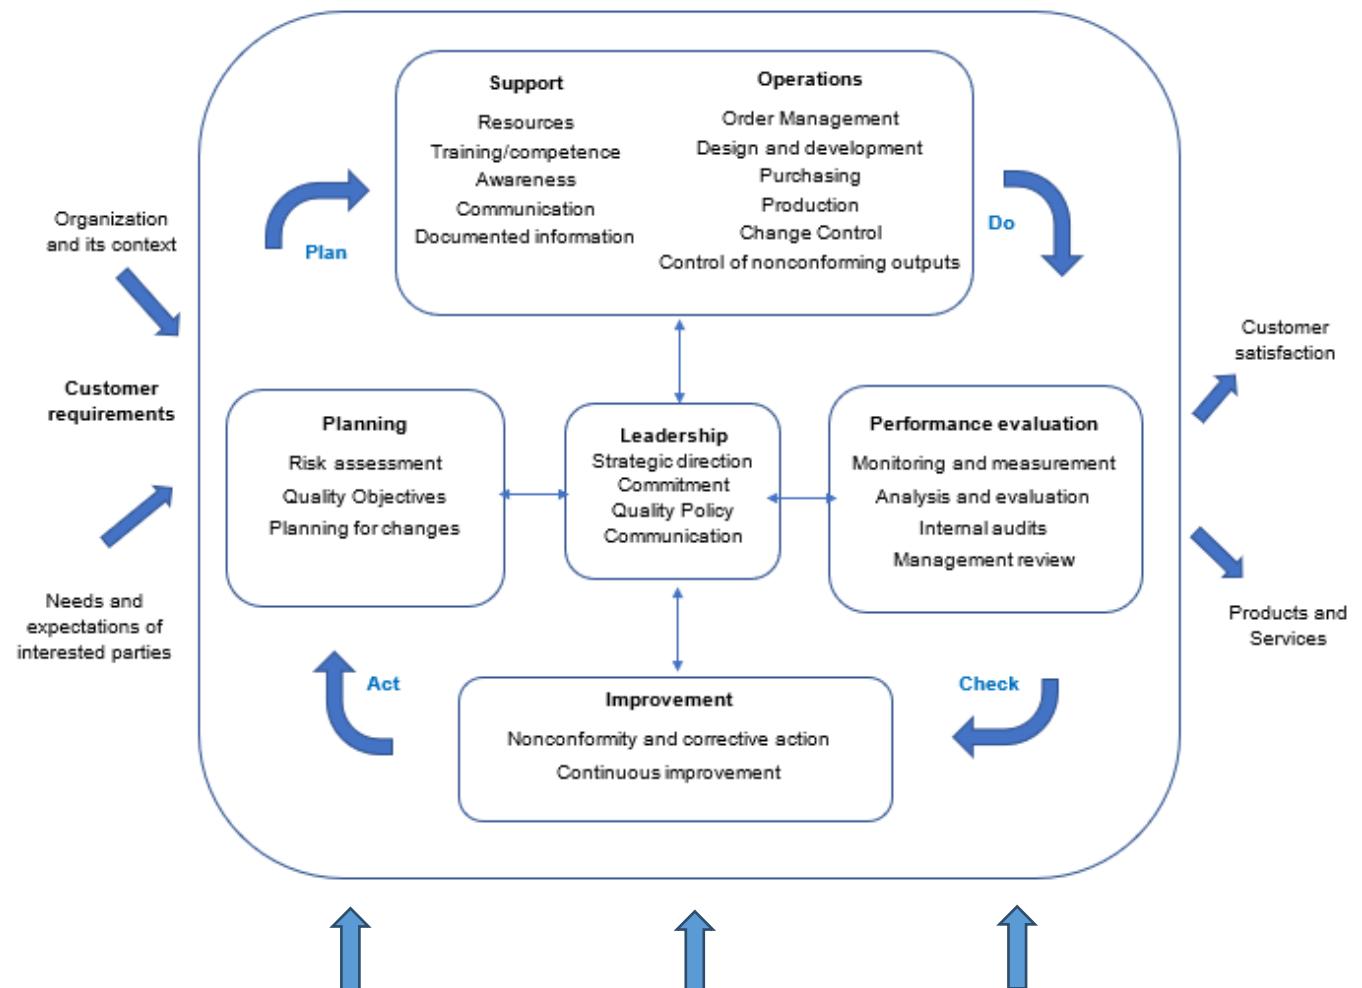

Q0003389 Fluke Corporate Quality Manual Rev. 130

1 Procedure Scope and Accessibility

This procedure applies to all personnel doing work under Fluke's control. Facilities may have supplementary policies, processes, and local procedures to further define their specific requirements and activities.

It is important to follow this policy to ensure Fluke's Quality Management System (QMS) is consistently implemented and followed to ensure compliance with all necessary standard, legal, regulatory and customer requirements.

This document does not contain confidential information and may be shared with personnel outside of Fluke and Fortive.

2 References

Internal

[80079-34 Ex Quality Manual \(Q0002115\)](#)

[Agile Program Management \(Q0000368\)](#)

[Control of Nonconforming Material Policy \(Q0000604\)](#)

[Corporate Training Policy \(Q000224\)](#)

[Corrective Action and Risk Mitigation Policy \(Q0001968\)](#)

[Document Control Policy \(Q0001697\)](#)

[Electrostatic Discharge Policy \(Q0002741\)](#)

[External Product Quality \(Q0000387\)](#)

[Fluke 17025 Quality Manual \(Q0002339\)](#)

[Fluke Corporate Scope and Context Statement \(Q0002401\)](#)

[Fluke Europe Quality Manual Addendum \(Q0000116\)](#)

[Fluke Supplier Quality Manual \(Q0002835\)](#)

[Fluke Warranty Administration Policy \(Q0002547\)](#)

[Internal Audit Process \(Q0001759\)](#)

[Management Review Policy \(Q0002464\)](#)

[Manufacturing Process Policy \(Q0002639\)](#)

[Measurement Management System \(Q0000405\)](#)

[QMS Records Retention Policy \(Q0002964\)](#)

[QMS Records Retention Policy](#): QMS Records Retention Requirements (Q0002689)

[Return Material Process \(RMA\) Policy \(Q0001228\)](#)

[Safety and Product Recall Process Policy \(Q0001963\)](#)

[Serialization Policy \(Q0002689\)](#)

External

ISO 9001 Quality Management Systems – Requirements

ISO/IEC 17025 General requirements for the competence of testing and calibration laboratories

ISO/IEC 80079-34 Explosive atmospheres – Application of quality systems for equipment manufacture

3 Terms and Definitions

None

4 Fluke Scope and Context

The overview of Fluke, its organization, context and interested parties as well as their needs and expectations are located in the [Fluke Corporate Scope and Context Statement](#). Each facility has a Scope and Context statement that further defines their context and interested parties based on the activities performed and products manufactured within that facility or functional area.

Fluke has established, maintains and continually improves our Quality Management System in accordance with the ISO 9001 standard, legal, regulatory and customer requirements.

As part of our Quality Management System, Fluke has determined the processes needed and their application throughout the company and:

- determines required inputs and expected outputs from these processes;
- defines the sequence and interaction of processes;
- establishes criteria and methods needed to ensure the effective operation and control of our processes;
- identifies the resources needed for these processes and ensures their availability and suitability;
- assigns the responsibilities and authority for these processes;
- addresses the risks and opportunities for improvement as determined in accordance with our planning processes;
- evaluates these processes and implements changes needed to ensure that these processes achieve their intended results;
- improves the processes and the Quality Management System.

To the extent necessary, Fluke maintains documented information necessary to support our processes and retains documented information as required to demonstrate that these processes are being carried out as planned.

5 Leadership

Leadership and Commitment

Top management demonstrates leadership and commitment with respect to the Quality Management System by:

- taking accountability for the effectiveness of the Quality Management System in achieving its intended results through active participation in management review;
- ensuring that the quality policy and quality objectives are established and are compatible with the strategic direction of Fluke;
- integrating the Quality Management System requirements with Fluke's business processes;
- promoting continuous improvement, the use of a process approach and risk-based thinking through use of our FBS tools;
- ensuring resources needed for the Quality Management System are available;
- communicating the importance of effective quality management and conforming to Fluke's Quality Management System requirements.

Top management demonstrates leadership and commitment with respect to customer focus by ensuring that:

- customer and applicable regulatory requirements are determined, understood, and consistently met;
- risks and opportunities that can affect conformity of products and services and the ability to enhance customer satisfaction are determined and addressed;
- focus on enhancing customer satisfaction is maintained through appropriate setting of performance objectives;
- customers have a method to provide quality feedback to Fluke.

Quality Policy

Top management has established [Fluke's Quality Policy](#) which is available in PLM and communicated throughout the company.

Roles and Responsibilities

Top management ensures that responsibilities and authorities for relevant roles are assigned, communicated and understood throughout Fluke. This is done through departmental organizational charts and job descriptions.

Top management has assigned the Director of Global Quality as the Management Representative with responsibilities that ensure:

- the Quality Management System conforms to the ISO 9001 standard requirements;
- the Quality Management System conforms to the ISO/IEC 17025 standard requirements as applicable for calibration laboratories accredited to ISO/IEC 17025;

- the Quality Management System conforms to the IEC 80079-34 standard requirements (accessed through the standards subscription service) as applicable for the manufacture of products intended for use in explosive atmospheres. See [Fluke 80079-34 Ex Quality Manual](#);
- processes are delivering their intended outputs;
- the performance of the Quality Management System is reported on and opportunities for improvements are identified;
- customer focus is promoted throughout Fluke;
- the integrity of the Quality Management System is maintained when changes are planned and implemented.

6 Planning

When planning for the Quality Management System, Fluke considers the context of the organization, its customers and their requirements and determines the risks and opportunities that need to be addressed in order to:


- give assurance that the Quality Management System can achieve its intended results;
- prevent or reduce undesirable effects and enhance desired effects;
- achieve improvement.

Fluke addresses these risks and opportunities by integration and implementation of actions into the Quality Management System and evaluation of the effectiveness of these actions through use of tools such as daily and visual management, Key Performance Indicator (KPI) bowlers and other measurement processes. Actions taken are proportional to the potential impact on the conformity of products and services.

Policy Deployment and Operational KPI reviews are used to establish objectives, measure performance and drive continuous improvement. Policy deployment is a structured process used by Fluke to focus on impactful, breakthrough objectives that are critical for achieving the strategic direction. The crucial cornerstones to achieving this success are the focus on the Voice of the Customer (VOC) and the planning process which links that focus to satisfying the innovation, delivery and cost objectives to meet customer needs.

Operations KPIs are defined and flowed to the relevant functions, levels and processes to measure the sustaining business processes. Improvement objectives are established as part of the annual planning process and Operations Reviews are held monthly to review results and countermeasures to misses, as necessary.

Policy Deployment Diagram

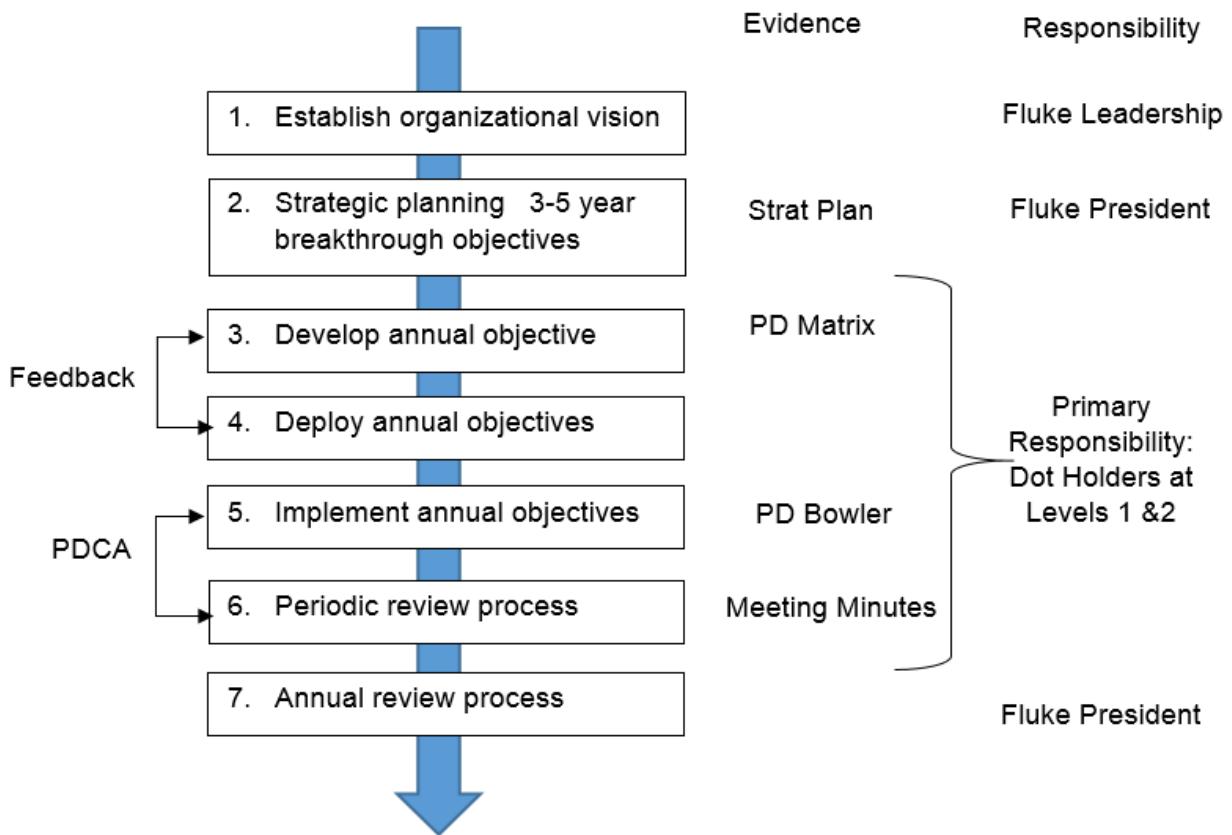

7 Support Resources

Fluke determines and provides the resources needed for the operation and improvement of the Quality Management System to ensure the products and processes achieve their planned results. When considering resources, Fluke considers the capabilities and constraints on existing resources as well as needs from external sources. Resources are determined and addressed at each facility and functional area. These may include:

- infrastructure;
- environment;
- materials and equipment;
- personnel.

Monitoring and Measurement Resources

Fluke provides the necessary equipment to ensure valid and reliable results are obtained when monitoring and measuring is used to verify the conformity of products and services.

Monitoring activities are defined in [Manufacturing Process Policy](#) and [Measurement Management System Policy](#) defines the policies, procedures and requirements of the Measurement Management System.

Competence and Awareness

Fluke determines the type and extent of training required for personnel performing work that affects the performance and effectiveness of its Quality Management System. Fluke provides training as necessary to meet these requirements.

Personnel are considered competent with respect to their assignment and/or job description, based on their education, training, skills, experience, and demonstrated results. Documented information as record of competence shall be retained in accordance with [Corporate Training Policy](#) and local process documents.

Personnel performing work under Fluke's control shall be aware of:

- the quality policy;
- relevant quality objectives;
- their contribution to the effectiveness of the Quality Management System;
- implications of not conforming to the Quality Management System.

Communications

Communication, both internal and external, is key to an effective Quality Management System and ensuring processes are followed and requirements are met.

Examples of communication include, but are not limited to:

- New and updated regulatory and statutory requirements
- Certifications and accreditations
- Communication of audit results (internal and external)
- Notification of changes to drawing, documents and procedures
- Resources needs
- Customer requests for information

Changes to products, processes and procedures are incorporated into the documents and communicated through the document management and ERP systems.

Newsletters, e-mails and SharePoint sites are also used to communicate information integral to the Quality Management System.

Guidance for responding to customer requests for information and standard Fluke responses are located on the [Serving Our Customers](#) SharePoint page on [Inside Fluke](#). Fluke certifications and registrations can be viewed and downloaded from the Fluke external websites.

Information on Fluke's communication and social media use policies can be found in the employee handbooks.

Documented Information

Fluke's Quality Management System includes documented information required by the ISO 9001 standard, as well information determined necessary by Fluke to ensure the effectiveness of the Quality Management System.

Fluke's document structure and the control of documents is defined in [Document Control Policy](#). This policy ensures documents are created in the acceptable formats with the necessary information to ensure proper control. Documented information is made available to all necessary personnel using control systems, such as PLM, and the use of links on SharePoint sites. These systems ensure only the current approved version of documented information is available to the users.

Retention of documented information (records) is defined in [QMS Records Retention Policy](#) and [QMS Records Retention Policy: QMS Records Retention Requirements](#) or the specific document. These procedures provide direction on how and where documented information is retained as well as the retention period and the disposition methods.

Organizational Knowledge

Fluke has identified and documented organizational knowledge that is necessary for the operation of its processes and to achieve conformity of products and services. Organizational knowledge is maintained by the functional groups and should be globally accessible through SharePoint sites or, at a minimum, should include a link to the knowledge system. As processes change, functional groups will determine whether additional information is necessary and if so, how it will be obtained.

8 Operations

Operational Planning and Control

Fluke plans, implements and controls processes needed to meet the requirements for the provision of products and services by:

- defining requirements for the products and services;
- establishing criteria for the processes and for the acceptance of the products and services;
- determining the resources needed to achieve conformity to the product and service requirements;
- implementing control of the processes in accordance with the criteria;
- developing, maintaining and retaining documented information to the extent necessary to demonstrate the conformity of products and services to their requirements.

[Manufacturing Process Policy](#) defines Fluke's manufacturing process policy and requirements.

Fluke controls changes to products and processes, including out-sourced processes, and reviews for unintended consequences of changes, taking action as necessary to mitigate any adverse effects.

Requirements for Products and Services

Fluke's communication with its customers includes:

- providing information relating to the products and services;
- responding to inquiries, contracts or orders, including changes;
- obtaining customer feedback relating to products and services, including customer complaints;
- handling or controlling customer property;
- establishing specific requirements for contingency actions, when relevant.

Fluke uses product development processes ([Agile Program Management Policy](#)) when determining the requirements for the products and services to be offered to customers, and ensures that:

- the requirements for the product and services are defined, including any applicable statutory and regulatory requirements;
- requirements considered necessary by Fluke are defined;
- Fluke can meet the claims for the product and services it offers.

Contract review ensures fulfillment of contract/order requirements, resolve any discrepancies, and coordinate the requirements with all affected areas of the company. The contract/order process includes quotations, order entry and subsequent contract/order changes.

As part of the quotation process, each department involved will communicate Fluke's terms of sale to the customer.

Before committing to supply product or services, Fluke reviews the contract/order to verify:

- requirements specified by the customer, including the requirements for delivery and post-delivery activities, such as routine service;
- requirements not stated by the customer but necessary for the specified or intended use, when known;
- requirements specified by Fluke;
- statutory and regulatory requirements applicable to the products and services;
- contract or order requirements differing from those previously expressed.

Fluke maintains records (electronic or hard copy) of the results of these reviews and on any new requirements for the products or services in accordance with local

process documents, [QMS Records Retention Policy](#) and [QMS Records Retention Policy: QMS Records Retention Requirements](#).

When the requirements for products and services change, Fluke ensures that relevant documented information is amended and that relevant persons are made aware of the changed requirements.

Design and Development of Products and Services

Fluke uses [Agile Program Management Policy](#) and the supporting processes, guidelines and checklists to control and verify the design (or redesign) of products to ensure that specified requirements are met. These processes ensure consistent and effective management of design activities in all divisions of Fluke.

Design and development activities include:

- determining the design input requirements relating to the product, including applicable statutory and regulatory requirements, and their identification, documentation and review;
- verification and validation of the design to ensure that the designed products meet all input requirements as well as performance, durability, reliability, serviceability, safety, regulatory, and contractual requirements.

All output documentation will be controlled and retained by the Project Manager as defined in the product development processes. At the end of the project, design disclosure drawings (e.g. drawings, component specifications, software, CAD databases) that are under Configuration Control, will be released in the approved Product Data Management (PDM) system.

Control of Externally Provided Processes, Products and Services

Fluke ensures that externally provided processes, products and services conform to requirements. Fluke determines the controls to be applied to externally provided processes, products and services when:

- products and services from external providers are intended for incorporation into Fluke's own products and services;
- products and services are provided directly to the customer(s) by external providers on behalf of Fluke;
- a process, or part of a process, is provided by an external provider as a result of a decision by Fluke.

Requirements for suppliers of materials are located in [Fluke Supplier Quality Manual](#).

Fluke determines and applies criteria for the evaluation, selection, monitoring of performance, and re-evaluation of external providers, based on their ability to provide processes or products and services in accordance with requirements. Fluke retains

Q0003389 Fluke Corporate Quality Manual Rev. 130

documented information of these activities and any necessary actions arising from the evaluations.

Fluke ensures that externally provided processes, products and services do not adversely affect its ability to consistently deliver conforming products and services to our customers.

Fluke ensures that externally provided processes remain within the control of its Quality Management System and defines both the controls that it intends to apply to an external provider and those it intends to apply to the resulting output.

Fluke takes into consideration the potential impact of the externally provided processes, products and services on Fluke's ability to consistently meet customer's requirements, applicable statutory and regulatory requirements and the effectiveness of the controls applied by the external provider.

Fluke determines the verification, or other activities, necessary to ensure that the externally provided processes, products and services meet requirements. Fluke ensures the adequacy of requirements prior to their communication to the external provider.

Using the purchase order, standard terms and conditions and [Fluke Supplier Quality Manual](#), Fluke communicates the following requirements to external providers:

- the processes, products and services to be provided;
- the approval of:
 - products and services;
 - methods, processes and equipment;
 - the release of products and services.
- competence, including any required qualification of persons;
- the external providers' interactions with Fluke;
- control and monitoring of the external providers' performance to be applied by Fluke;
- verification or validation activities that Fluke, or our customer, intends to perform at the external supplier's premises.

Fluke retains documented information of these activities and any necessary actions arising from evaluations in accordance with [QMS Records Retention Policy: QMS Records Retention Requirements](#).

Product and Service Provision

Production, installation, support and servicing processes that directly affect quality have been identified and planned to ensure those processes are carried out under controlled conditions that include:

Q0003389 Fluke Corporate Quality Manual Rev. 130

- the availability of documented information that defines the characteristic of the products/services and the results to be achieved.
- the availability of work instructions and procedures;
- the availability and use of suitable equipment;
- the implementation of monitoring and measurement devices at appropriate stages in the process with acceptance criteria;
- the use of suitable infrastructure and environment;
- the appointment of trained and competent persons, including any required qualifications;
- the validation, and periodic revalidation, of the ability to achieve planned results where the resulting output cannot be verified by subsequent monitoring or measurement;
- where possible the implementation of error-proofing (poka-yoke) activities;
- documented information for the release, delivery and post-delivery activities where required.

Calibration and repair services are provided for all our instruments that have guaranteed performance specifications as well as for a wide range of instruments manufactured by other companies. The service centers have established processes and procedures to ensure these activities are carried out under controlled conditions. Calibration and repair services are the responsibility of our service organization.

Fluke has a network of strategically located service centers which provide:

- Repair services;
- Calibration services;
- Upgrade services;
- Service agreements;
- Extended warranty agreements;
- Asset management agreements.

Service centers also provide warranty failure data to the factory for the purpose of monitoring product failure trends.

All Fluke calibration services are in compliance to [Measurement Management System Policy](#). Where appropriate, accredited calibration activities are provided in accordance with [Fluke 17025 Quality Manual](#).

The Service Parts department maintains replacement parts and manual inventory for Fluke service centers and direct parts sales to customers. All replacement parts are subjected to the same inspection and quality assurance programs applicable to parts used in production.

A product exchange service provides rebuilt assemblies for self-maintenance customers, fast turn-around-time and low-cost products and accessories.

Identification and Traceability

Fluke defines its part marking and traceability requirements in [Serialization Policy](#).

Records are established and maintained providing evidence the product has been inspected and/or tested. These records identify the person responsible for the release of the conforming products.

Process owners ensure the inspection and test status of products are identified by indicating conformance or nonconformance by using stamps, labels and/or physical locations. This identification is maintained and understood, as defined in local work instructions, throughout production, installation and servicing of products to ensure only products that have passed the required inspections and tests are shipped, used or installed. All departments are responsible for complying with [Control of Nonconforming Material Policy](#) and for taking corrective action as appropriate per [Corrective Action and Risk Mitigation Policy](#).

Customer and External Provider Property

Fluke identifies customer property as “product and accessories” returned for repair or calibration. Fluke does not use any other type of customer or provider property.

Fluke identifies customer property upon receipt and exercises care to prevent damage. In the event a customer’s property is damaged or lost, Fluke reports this to the customer and takes action to address the situation.

Preservation

Fluke has implemented local processes for the handling and preservation of product as necessary in order to prevent damage and deterioration.

Materials and stores departments are responsible for establishing processes for purchased parts. Production departments are responsible for establishing processes for work in process. The distribution centers are responsible for establishing processes for shipping product to the customer.

All organizations handling printed circuit assemblies (PCAs) shall comply with [Electrostatic Discharge Policy](#).

Post-delivery Activities

Fluke determines and meets requirements for post-delivery activities related to its products and services. In determining post-delivery activities, Fluke considers:

- statutory and regulatory requirements;
- potential undesired consequences associated with its products and services;
- the nature, use and intended lifetime of our products and services;
- customer requirements;
- customer feedback.

Requirements for post-delivery activities are met through Fluke's:

- **Warranty Management:** The [Fluke Warranty Administration Policy](#) demonstrates structured and compliant post-delivery warranty processes. This ensures consistent handling of in-warranty instruments by customer service, by providing:
 - **RMA Scrap Management:** The [Return Material Process \(RMA\) Policy](#) ensures traceability, customer communication, and appropriate credit issuance or scrapping of returned items.
 - **Onsite Service:** On-site service is a specific activity available for purchase and is not considered a post-delivery activity. Refer to [Fluke Warranty Administration Policy](#) for more details.
 - **Recall Process:** The [Safety and Product Recall Process Policy](#) establishes a comprehensive framework for managing post-delivery safety and recall activities. This includes:

Control of Changes

Fluke reviews and controls changes for production and service provisions, to the extent necessary to ensure continuing conformity with applicable requirements. Fluke retains documented information on these changes and the person(s) authorizing the change as well as any necessary actions arising from the review.

Release of Products and Services

Fluke has planned checks at appropriate stages in production and service to verify that requirements have been met. Products are not released to the customer until the planned checks have been successfully completed unless otherwise approved by the relevant authority, and where required by the customer.

Documented information is retained providing evidence the product has been inspected and/or tested. Records identify the inspection and test authority responsible for the release of conforming products.

Control of Nonconforming Outputs

Fluke ensures that outputs that do not conform to their requirements are identified and controlled to prevent their unintended use or delivery through local processes as defined in [Control of Nonconforming Material Policy](#) for materials or [Fluke 17025 Quality Manual](#) for ISO/IEC 17025 accredited calibration processes.

Fluke takes appropriate actions based on the nature of the nonconformity and its effect on the conformity of products and services determined at our facilities and after delivery or service as defined in [Corrective Action and Risk Mitigation Policy](#).

Fluke retains documented information that describes the nonconformity, describes the actions taken, describes any concessions obtained and identifies the authority deciding the actions.

9 Performance Evaluation

Monitoring, Measurement, Analysis and Evaluation

During new product development, or when an existing product design change is required, the responsible engineering organization will determine the measurements to be made, the accuracy required, the frequency of the measurement and will select the appropriate inspection, measuring, and test equipment that is capable of the necessary accuracy and precision.

Test systems are defined as any hardware or software used in production or service to verify the acceptability of the product or service. Test systems will be validated prior to their initial use and whenever a product or test system requires a change that could affect the acceptability of the product or service. Test system use, validation, maintenance and control will be described in local work instructions.

Where the results of processes cannot be fully verified by subsequent inspection and testing of the product and where processing deficiencies may become apparent only after the product is in use, the processes shall be carried out by qualified operators and/or shall require continuous monitoring and control of process parameters to ensure the specified requirements are met.

The requirements for qualification of process operations, including associated equipment and personnel shall be specified.

Supervisors/process owners are responsible for in-process and final inspection, testing, and monitoring per documented work instructions and design control information. Equipment maintenance documentation will list all equipment in the process owner's area of responsibility, maintenance schedules, maintenance instructions, and training records for all personnel performing maintenance.

Customer Satisfaction

Fluke monitors customer satisfaction through surveys, data collected through the External Product Quality Database, and the customer feedback system as defined in local process documents.

Analysis and Evaluation

Measuring and monitoring of processes and process outputs are used to determine the effectiveness of various processes as appropriate. These measurements also roll-up to strategic goals related to, among other things, the Core Value Drivers of Core Growth, Operating Margin Expansion (OMX) and Quality. The goals are documented in the policy deployment matrices and/or KPI bowlers at the top, divisional and departmental levels of the company. Countermeasures will be written for corrective action as determined by top management.

The results of analysis are used to evaluate:

- conformity of products and services;

- the degree of customer satisfaction;
- the performance and effectiveness of the Quality Management System;
- whether planning has been implemented effectively;
- the effectiveness of actions taken to address risks and opportunities;
- the performance of external providers;
- the need for improvements to the Quality Management System.

Internal Audits

[Fluke Global Audit Policy](#) defines Fluke's internal audit policy and program for verifying the Quality Management System has been effectively implemented and that processes conform to internal requirements and ISO standard requirements.

Frequency of audits, selection of auditors and corrective action requirements are defined in [Fluke Global Audit Policy](#).

Management Review

Fluke performs Management Review on different levels throughout the year according to processes defined by the Fortive Business System including Policy Deployment, Monthly Operating Reviews, and Daily and Visual Management. Over the course of the year, a complete Management Review is performed involving the L1 and L2 managers.

Management Review inputs include:

- status of actions from previous Management Reviews;
- changes in external and internal issues that are relevant to Fluke's Quality Management System;
- information on the performance and effectiveness of Fluke's Quality Management System including:
 - customer satisfaction and feedback from relevant interested parties;
 - the extent to which quality objectives have been met;
 - process performance and conformity of products and services;
 - nonconformities and corrective actions;
 - monitoring and measurement results;
 - audit results;
 - the performance of external providers;
 - equipment intended for use in explosive atmospheres, as applicable.
- adequacy of resources;
- effectiveness of actions taken to address risks and opportunities;
- opportunities for improvement.

Management Review outputs include decisions and actions related to:

- opportunities for improvement;

- any need for changes to the Quality Management System;
- resource needs.

Fluke Corporate Management Review records are defined in [Management Review Policy](#). Records for Management Reviews performed at other levels within Fluke may be in the same format, PowerPoint presentations or other suitable records and shall be retained in accordance with [QMS Records Retention Policy: QMS Records Retention Requirements](#).

10 Improvement

Continuous Improvement

Fluke continuously improves the suitability, adequacy and effectiveness of our Quality Management System through the use of Fortive Business System (FBS). FBS uses trained personnel (FBS champions) and tools such as problem solving and Kaizen activities.

Improvement opportunities include:

- improving products and processes to better address customer needs and expectations;
- correcting or preventing undesired effects;
- improving the effectiveness of the Quality Management System.

Nonconformances and Corrective Actions

Fluke takes action to address nonconformances, correct or control the situation and address the consequences at a level that is appropriate for each nonconformance. Records of the nonconformance, actions taken and the results are created and maintained in accordance with [Control of Nonconforming Material Policy](#) and [Corrective Action and Risk Mitigation Policy](#).

The need for taking action to eliminate the cause is evaluated by reviewing and analyzing the nonconformity, determining the cause and determining whether similar situations can or do exist.

Fluke implements actions as needed and reviews the effectiveness of the actions taken. If necessary, risks and opportunities for this product or service are evaluated and updated and, if required, changes are made to the Quality Management System.

Corrective action policies are further defined in [External Product Quality Policy](#) and [Corrective Action and Risk Mitigation Policy](#).

11 Approvals and Notifications

Process Owner/Approver:

Director of Global Quality


Document Author/Approver:

Quality Systems Manager

Document Reviewer:

Corporate Quality Council

ALL changes to this policy document MUST BE communicated to all Fluke labs, service centers, production areas and the Corporate Quality Council members for awareness. The revision of the Quality Manual is referenced on statements of calibration and on customer purchase orders for service and the revisions must match.

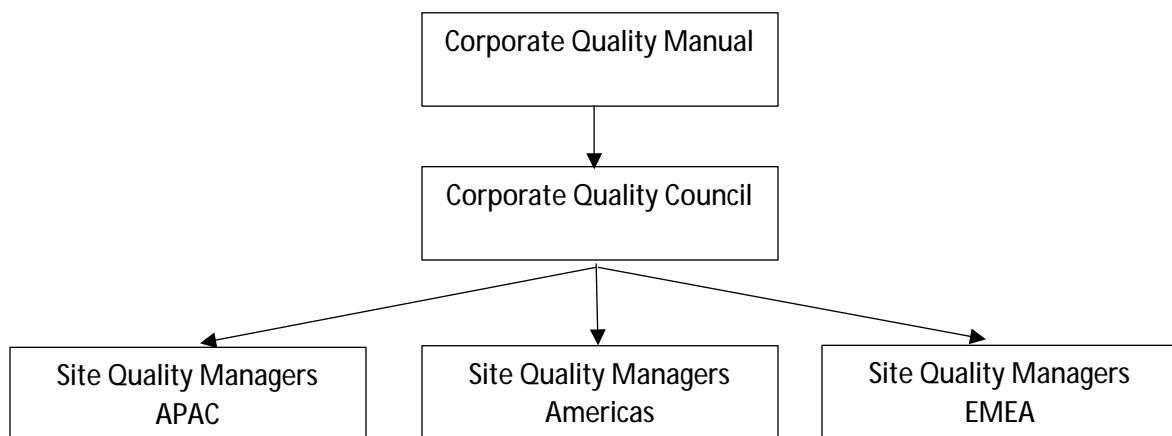

Q0003389 Fluke Corporate Quality Manual Rev. 130**12 Change History** (all but last 3 revisions are hidden)

The translated version of this document must be reviewed and revised each time this document is revised to ensure changes area easily identified for translation purposes.

Revision Date	Brief Description of Change(s)	Training required (Y/N)
Rev 128 Aug 2024	Revision canceled in PLM because of DCO-000871 issue, which took revision 128. No changes were made during revision 128. Revisions made on revision 129.	No
Rev 129 Aug 2024	Updated document links / references and formatted per new template, removed “appendix A” from document title (Q0002689) – Updated Section 11 Approvals and Notifications section to include additional information regarding communication of changes (CANA-0078) and made Quality Systems Manager Author/Approver, rather than listing twice. Added accessibility statement to Section 1.	No
Rev 130 AUG 2025	Updated public links to the new URL provided by the web services team. Update to the Post Delivery Activities section to further define how Fluke adheres to this portion of ISO9001 requirements.	No

End of Doc